

FIG. 1

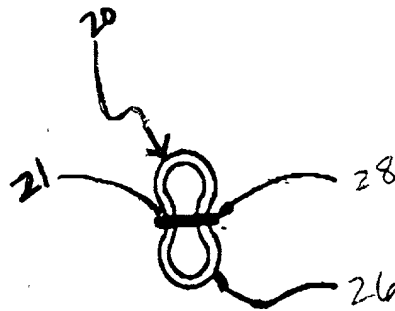


FIG. 2

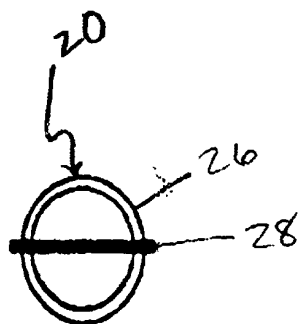



Fig. 3

0991407, 11501



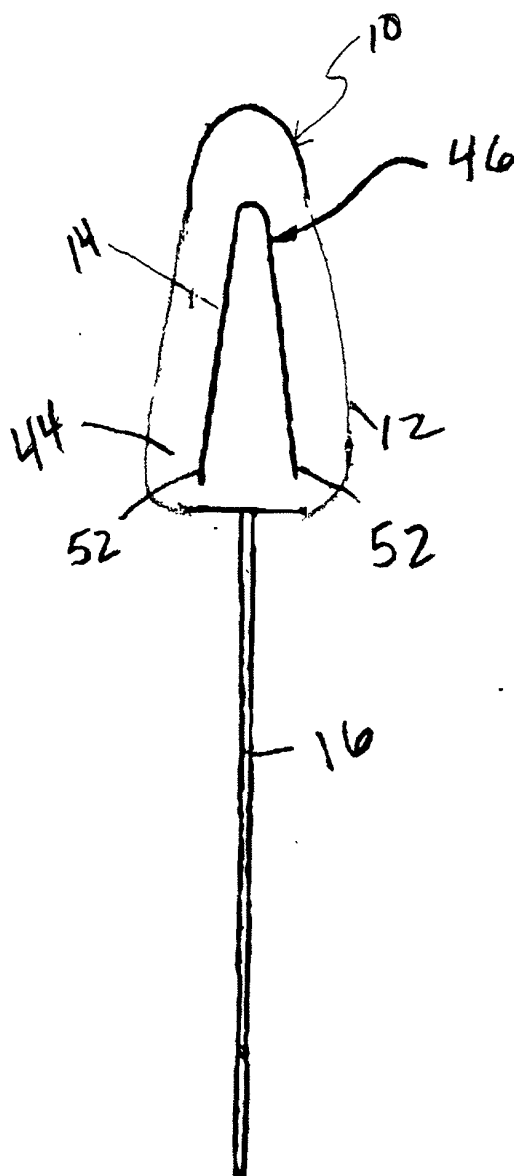


Fig. 5

FIG. 5

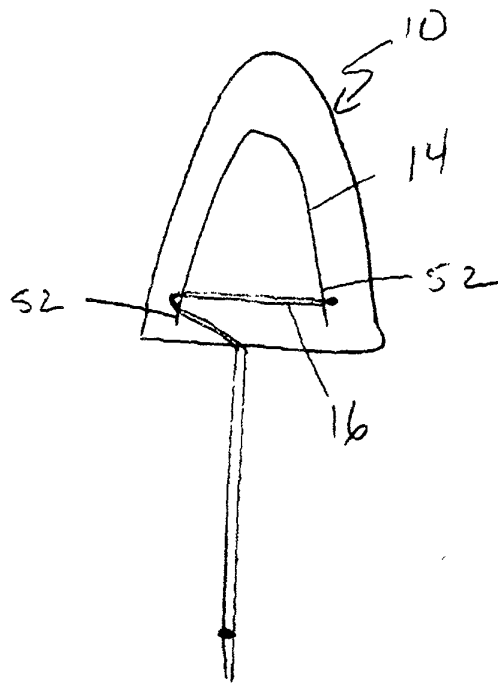


FIG. 5a

09091407 11501

"Catamenial Device Change Indicator"

Anthony DiSalvo, et al.

Docket No. PPC-812

09091407 11501

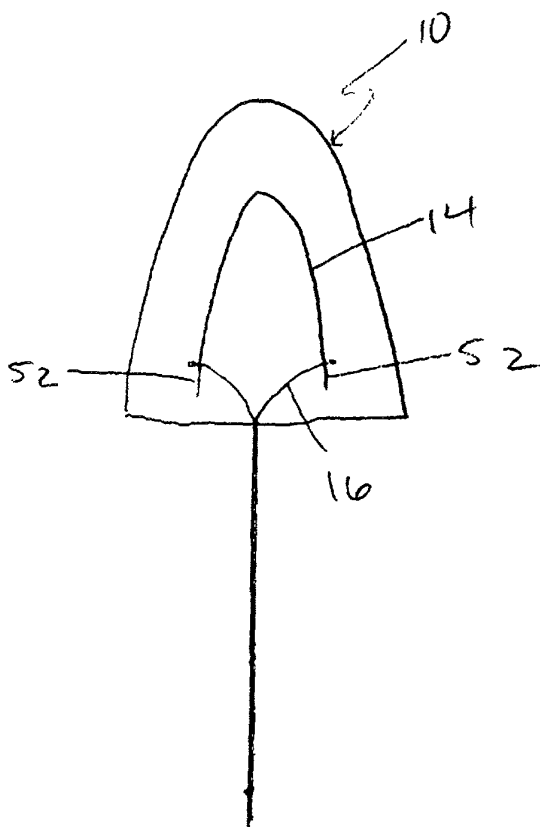


Fig. 5b

"Catamenial Device Change Indicator"

Anthony DiSalvo, et al.

Docket No. PPC-812

FIG. 5 C

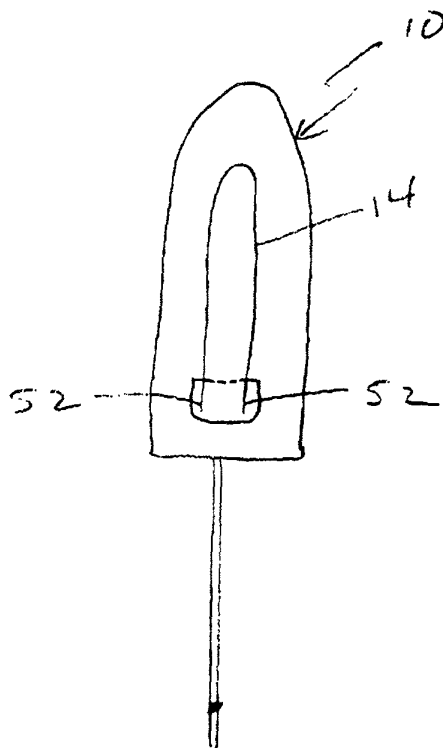


FIG. 5 C

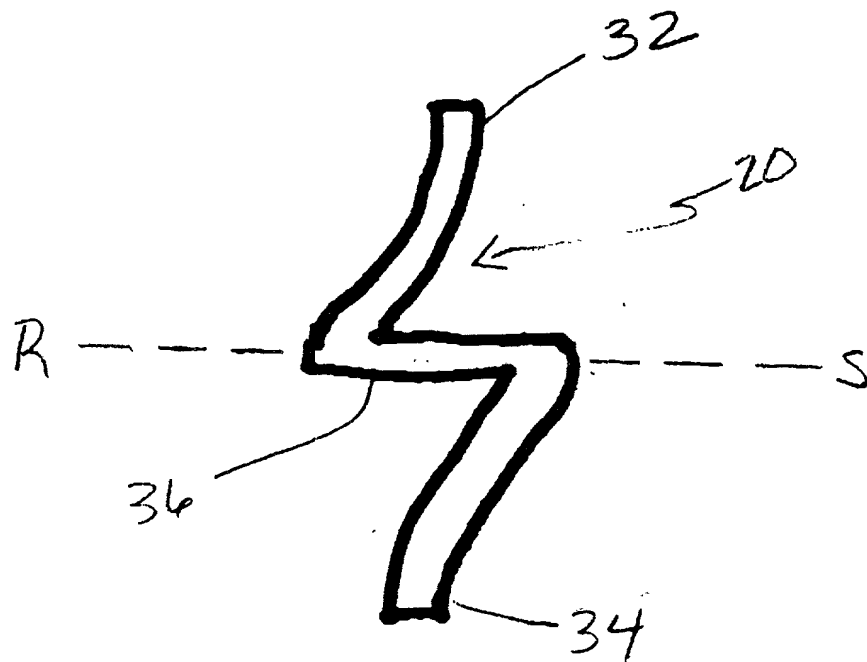


FIG. 6

FIG. 6

"Catamenial Device Change Indicator"

Anthony DiSalvo, et al.

Docket No. PPC-812

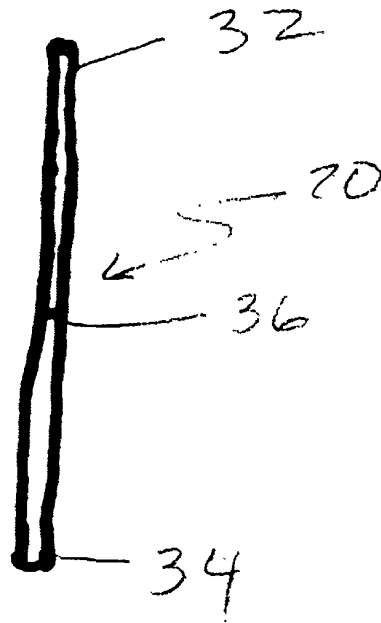


FIG. 7


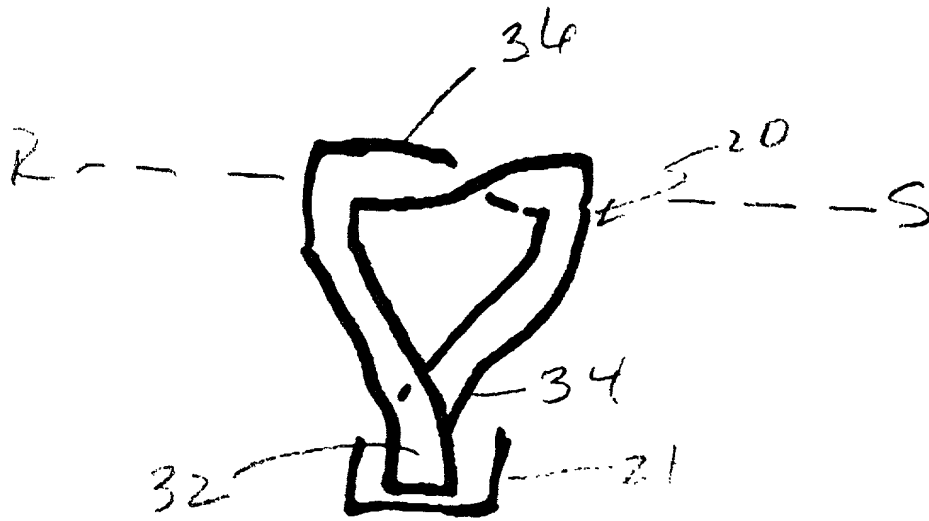


Fig. 8

09931407, 111601
109777 2046660

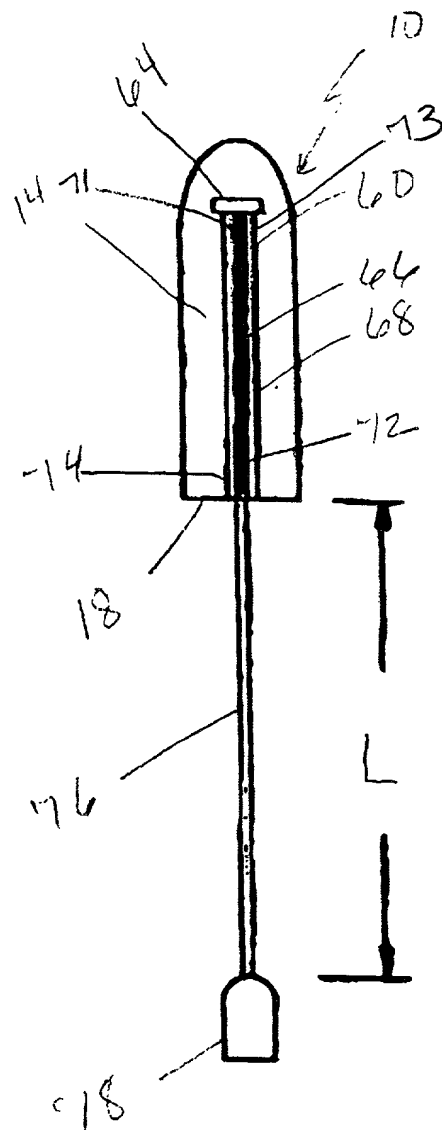

F16.9

"Catamenial Device Change Indicator"

Anthony DiSalvo, et al.

Docket No. PPC-812

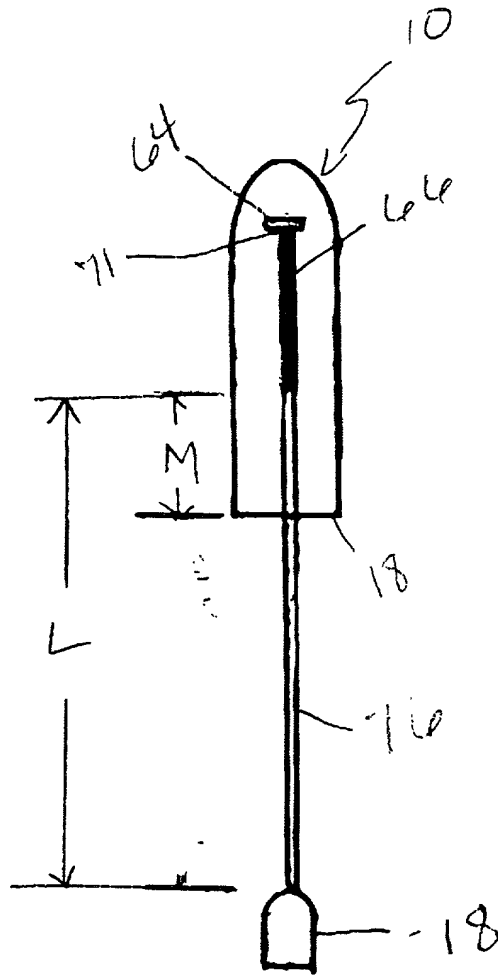


Fig. 16. 10

09931407.111601

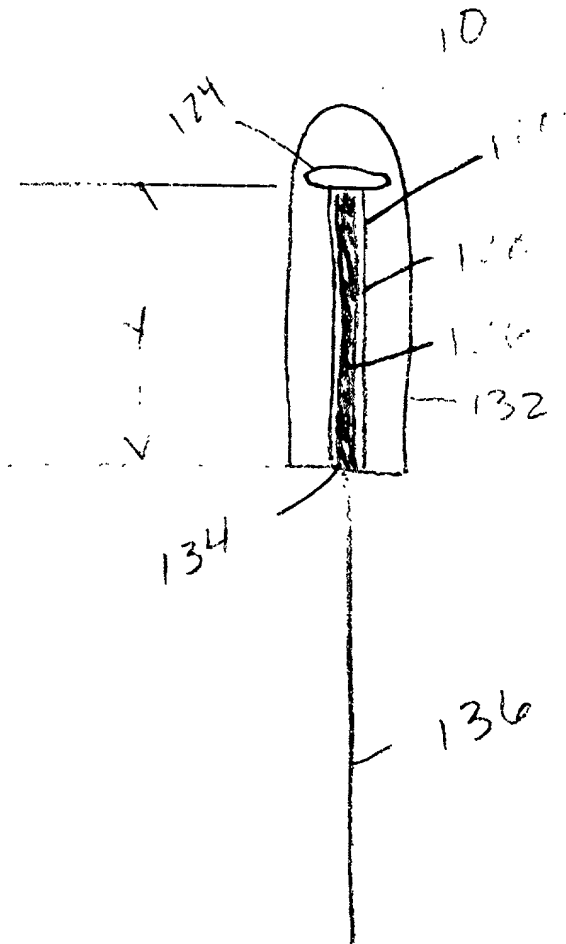


Fig. 11

0091407-11501

"Catamenial Device Change Indicator"

Anthony DiSalvo, et al.

Docket No. PPC-812

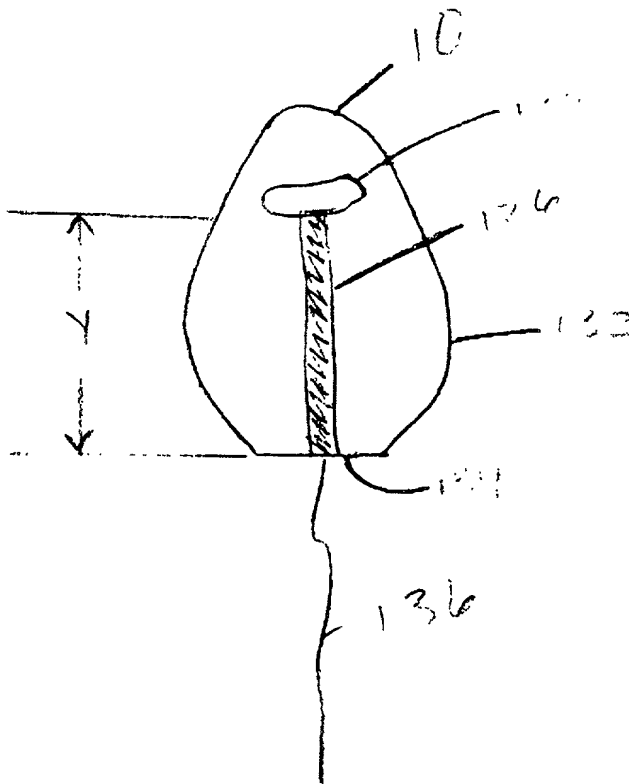


Fig. 12

PPC-812-116.12

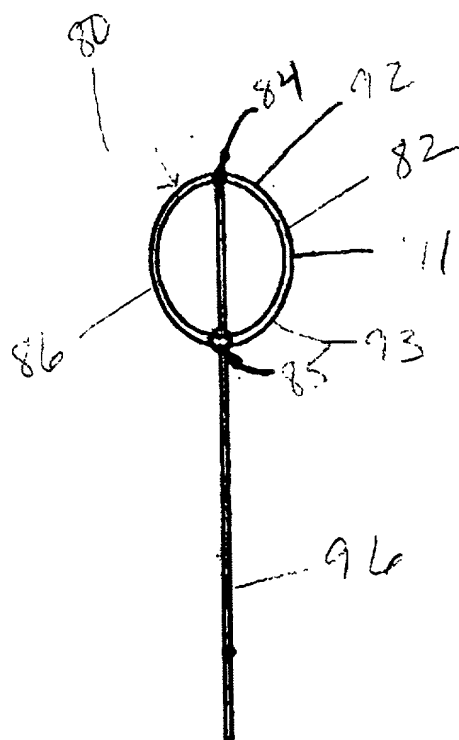


FIG. 13

09991467, 111601

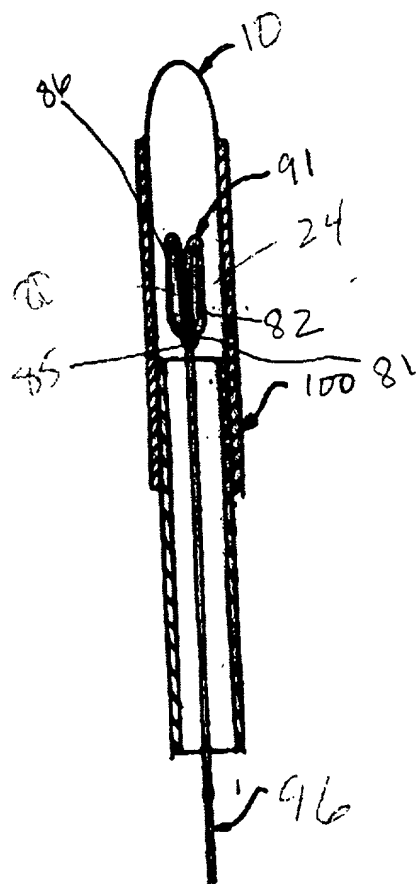


FIG. 14

FIG. 14

"Catamenial Device Change Indicator"

Anthony DiSalvo, et al.

Docket No. PPC-812

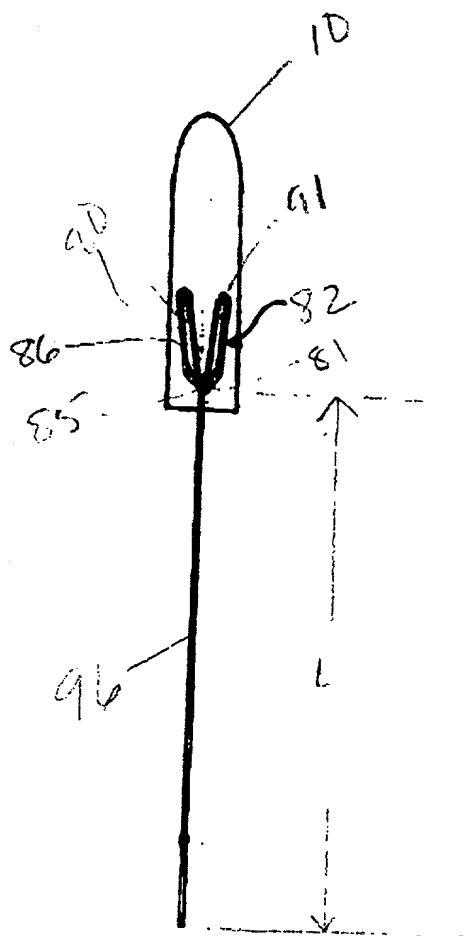


FIG. 15

"Catamenial Device Change Indicator"

Anthony DiSalvo, et al.

Docket No. PPC-812

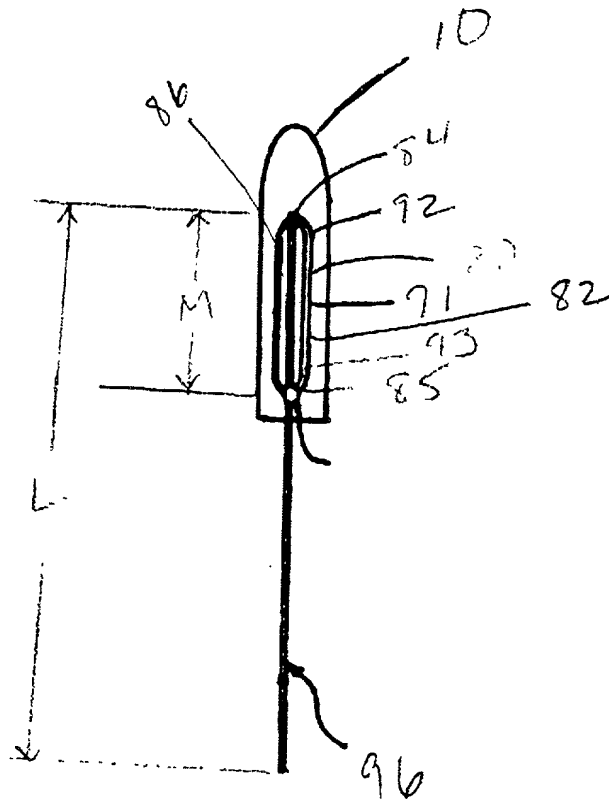


FIG. 16

09991407.111601

"Catamenial Device Change Indicator"

Anthony DiSalvo, et al.

Docket No. PPC-812

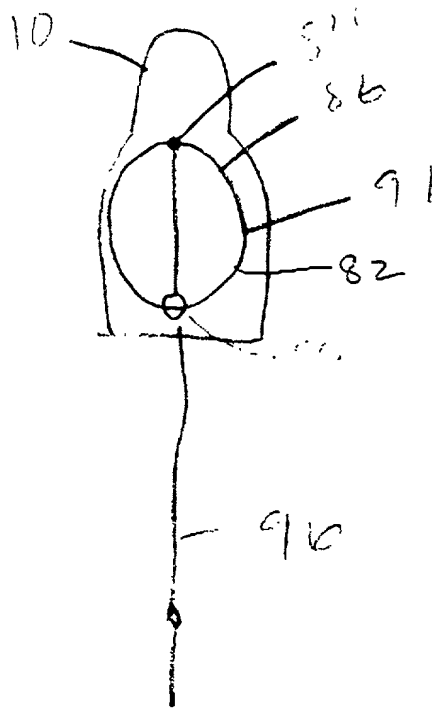


Fig. 17

00001407-11501